

FIG. 1

APPLICANT: NEUMILLER ET AL.
TITLE: HAZARD MITIGATION IN MEDICAL DEVICE
ATTORNEY/AGENT: STEVEN J. SHUMAKER
REG. NO. 36,275 TELEPHONE: 651.735.1100
DOCKET NO.: 1023-029US01 SHEET 1 OF 3

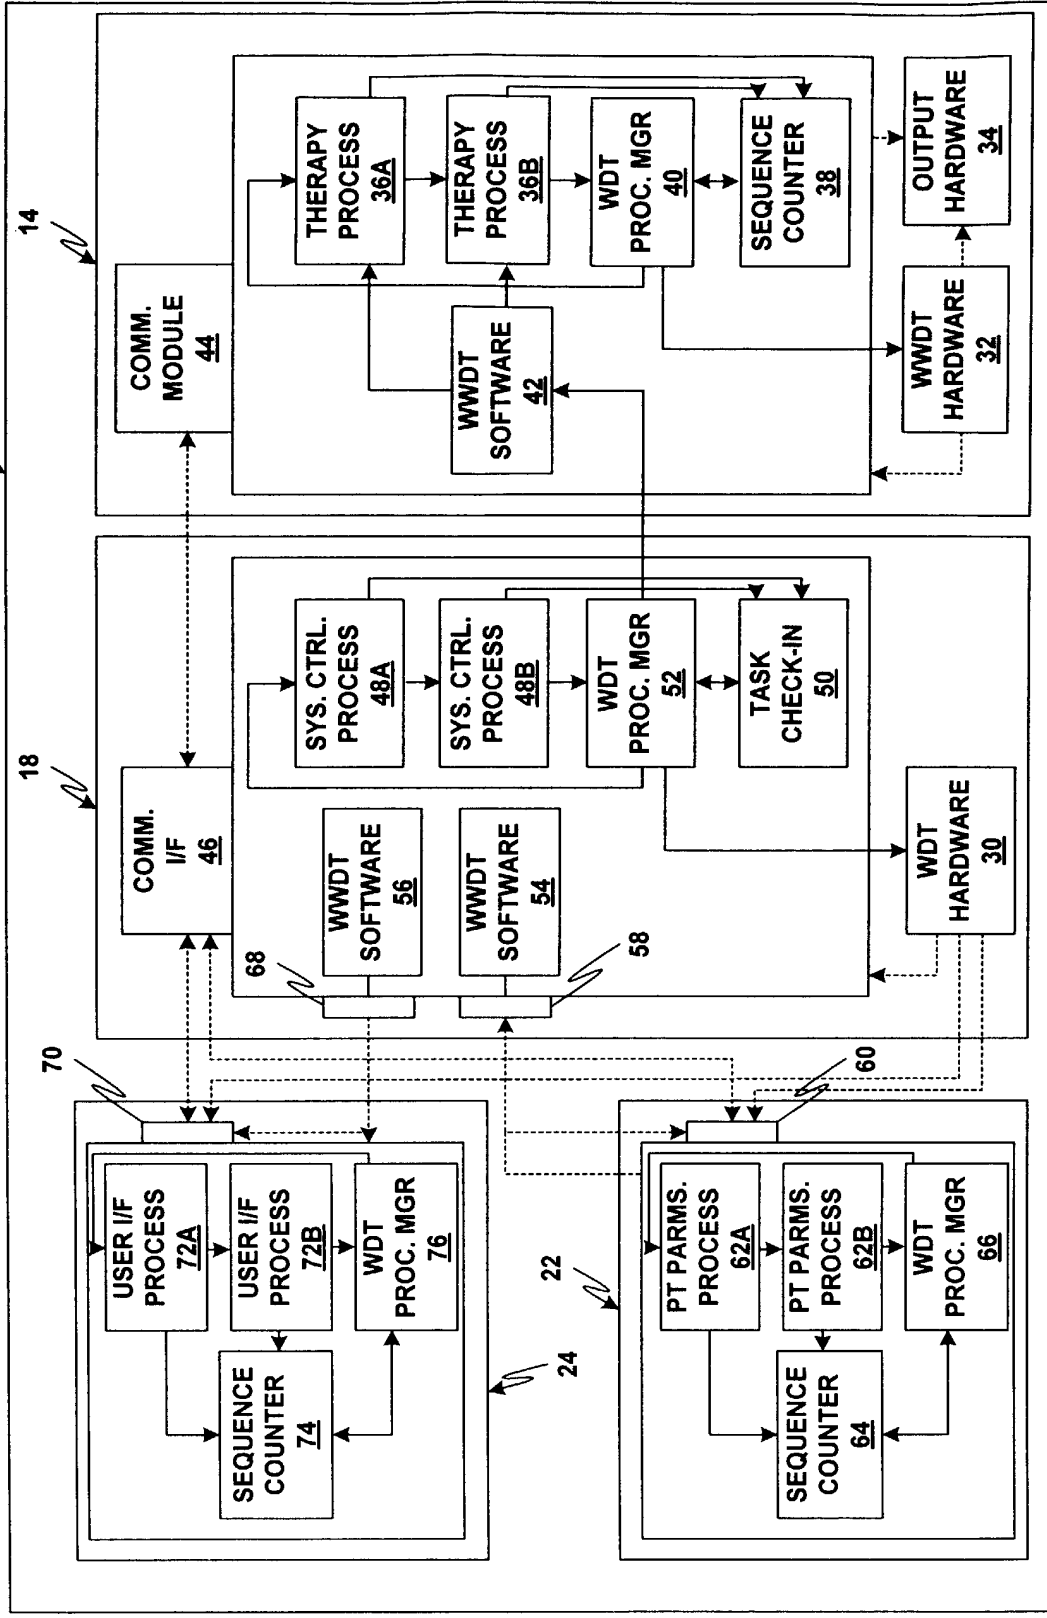


FIG. 2

PLICANT: NEUMILLER ET AL.
TITLE: HAZARD MITIGATION IN MEDICAL DEVICE
ATTORNEY/AGENT: STEVEN J. SHUMAKER
REG. NO. 36,275 TELEPHONE: 651.735.1100
DOCKET NO.: 1023-029US01 SHEET 2 OF 3

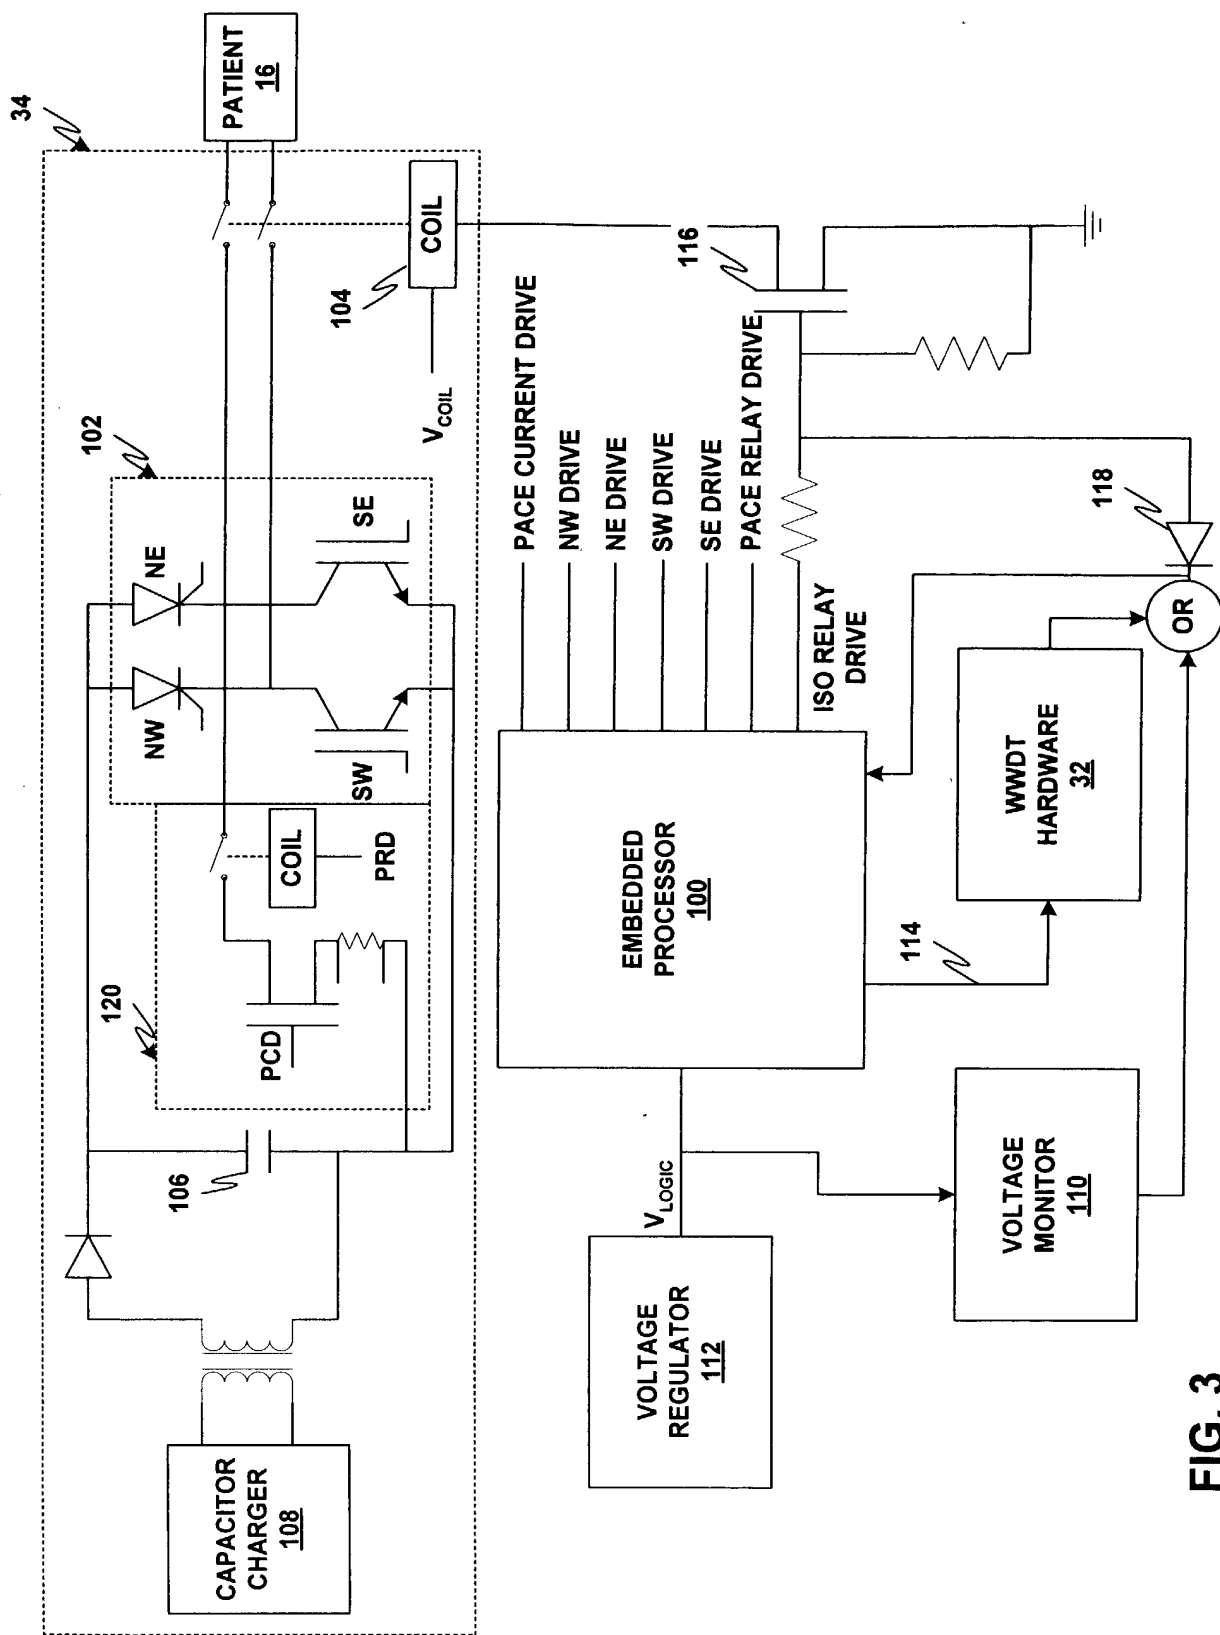


FIG. 3